




MitraClip™ G4 System

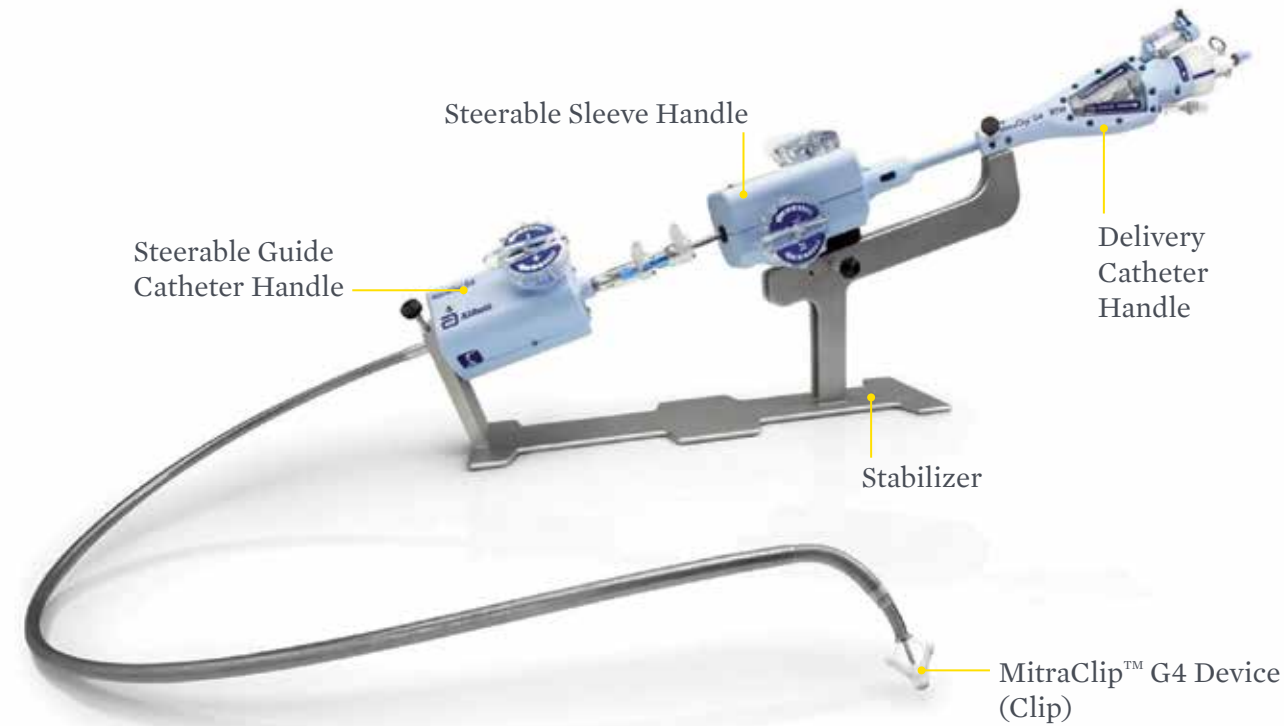


MITRACLIP™ G4 DEVICE CLOSE-UP

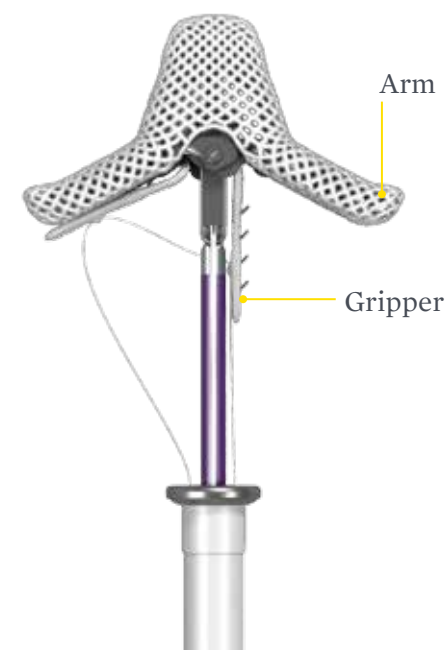

DELIVERY CATHETER HANDLE CLOSE-UP

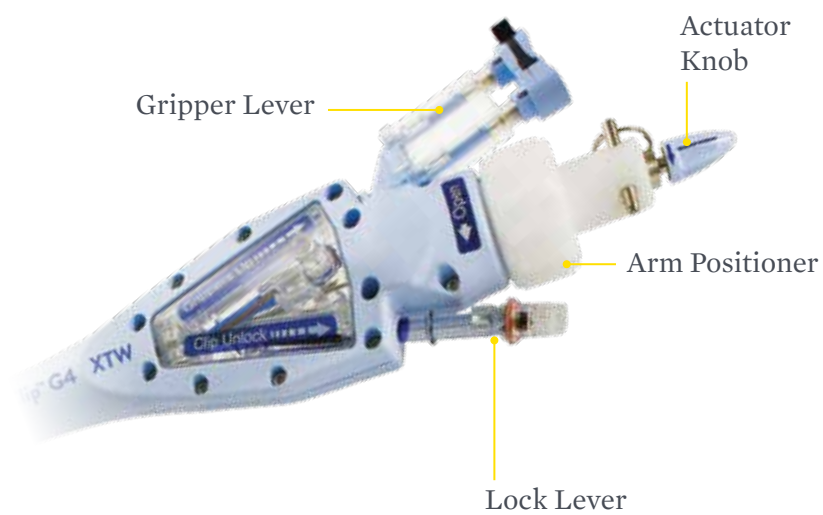

CAUTION: This product is intended for use by or under the direction of a physician. Prior to use, reference the Instructions for Use, inside the product carton (when available) or at efu.abbottvascular.com or at medical.abbott/manuals for more detailed information on Indications, Contraindications, Warnings, Precautions and Adverse Events. Information contained herein for DISTRIBUTION in Australia and New Zealand ONLY. Illustrations are artist's representations only and should not be considered as engineering drawings or photographs. Abbott Medical Australia Pty Ltd, 299 Lane Cove Road, Macquarie Park, NSW 2113 Ph: 1800 839 259 Abbott Medical New Zealand Ltd, Ground Floor, Bldg D, 4 Pacific Rise, Mount Wellington, Auckland 1060 Ph: 0800 656 233 W: www.cardiovascular.abbott E: ANZStructuralHeart@abbott.com ©2021 Abbott. All rights reserved. MAT-2103744 v1.0 | Item approved for ANZ use only





MitraClip™

Transcatheter Mitral Valve Repair

GUIDE

PROCEDURAL POSITIONING AND IMAGING

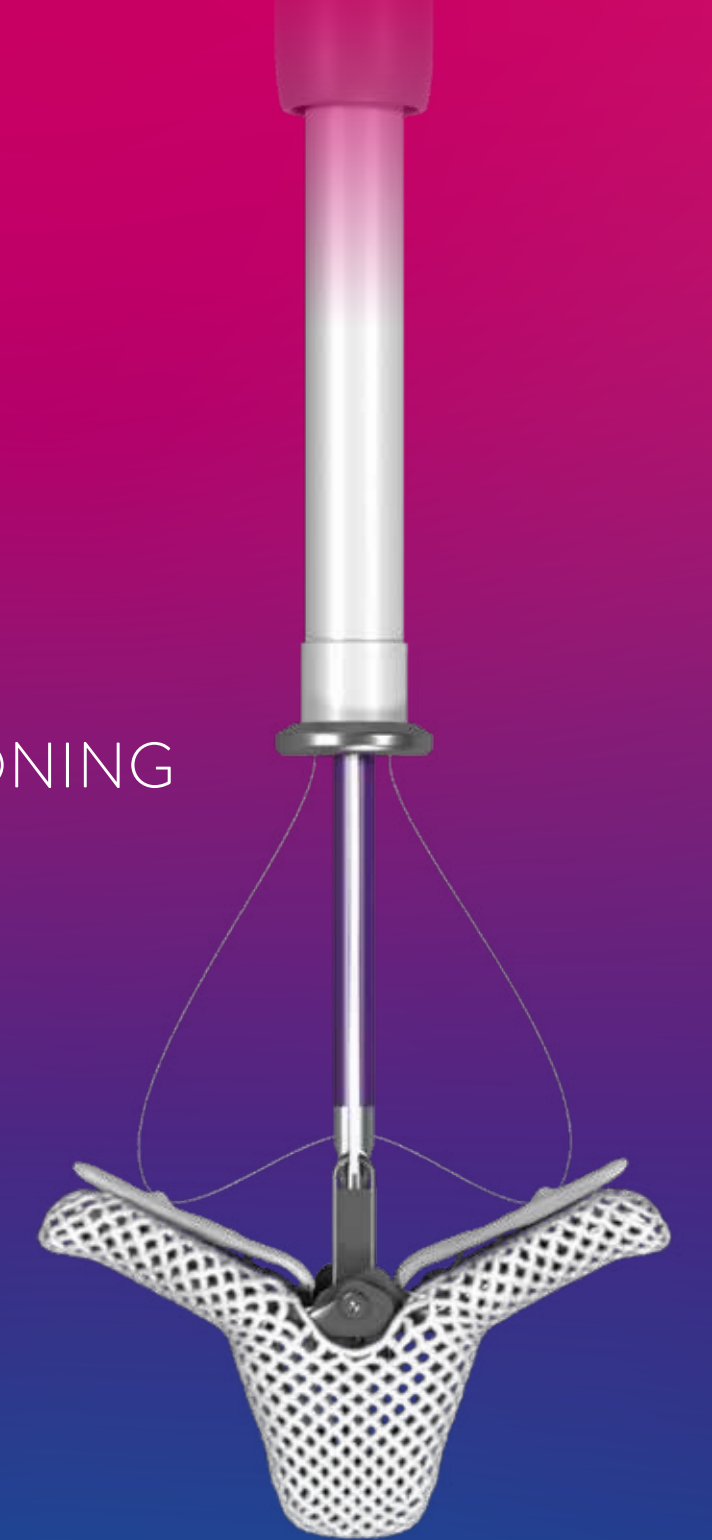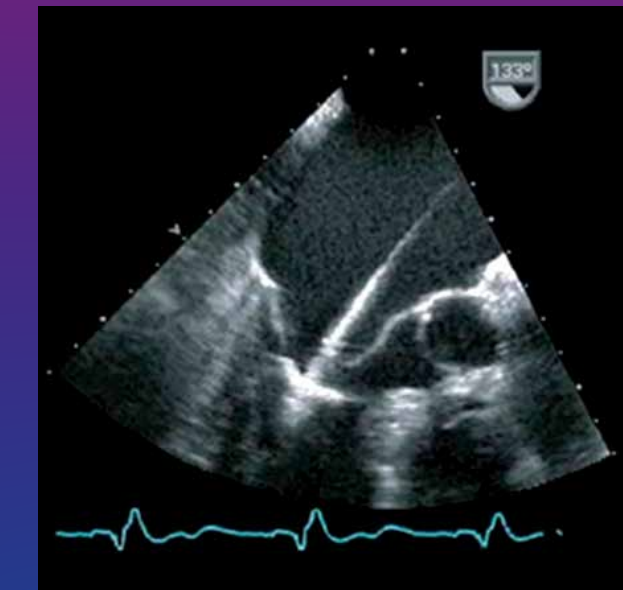

This material may be utilized for Clinical Site participants involved in Abbott sponsored trials or disclosed to a user facility for educational purposes.


Information contained herein for **DISTRIBUTION outside in Australia and New Zealand ONLY.**

©2021 Abbott. All rights reserved. MAT-2005413 v1.0 | Item approved for ANZ use only.




PROCEDURAL POSITIONING AND IMAGING GUIDE


CLIP DELIVERY SYSTEM COMPONENTS

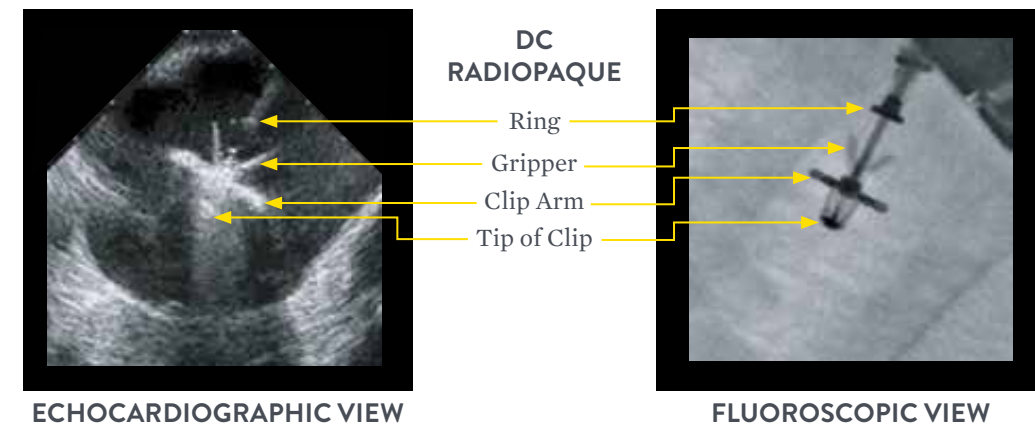


TRANSSEPTAL

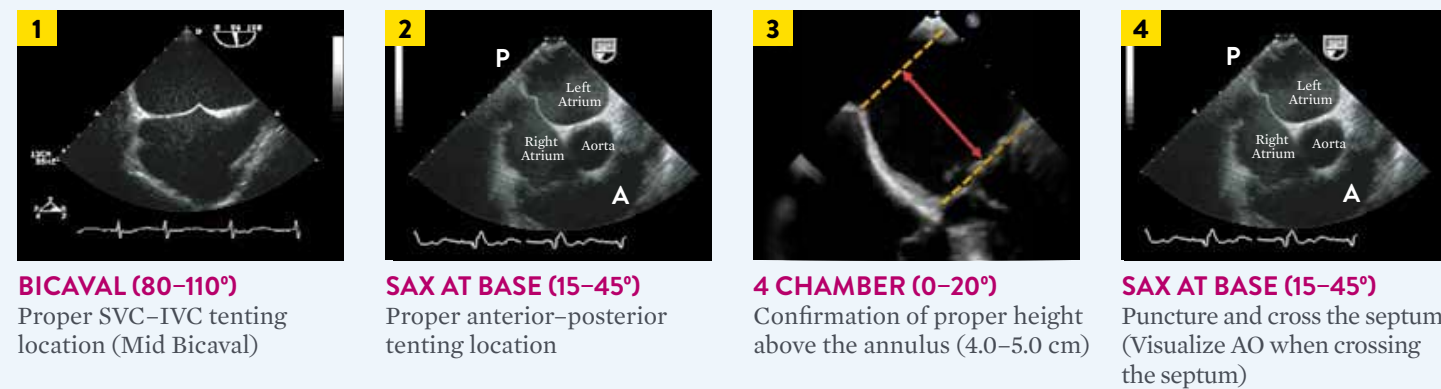

POSITIONING AND TRAJECTORY

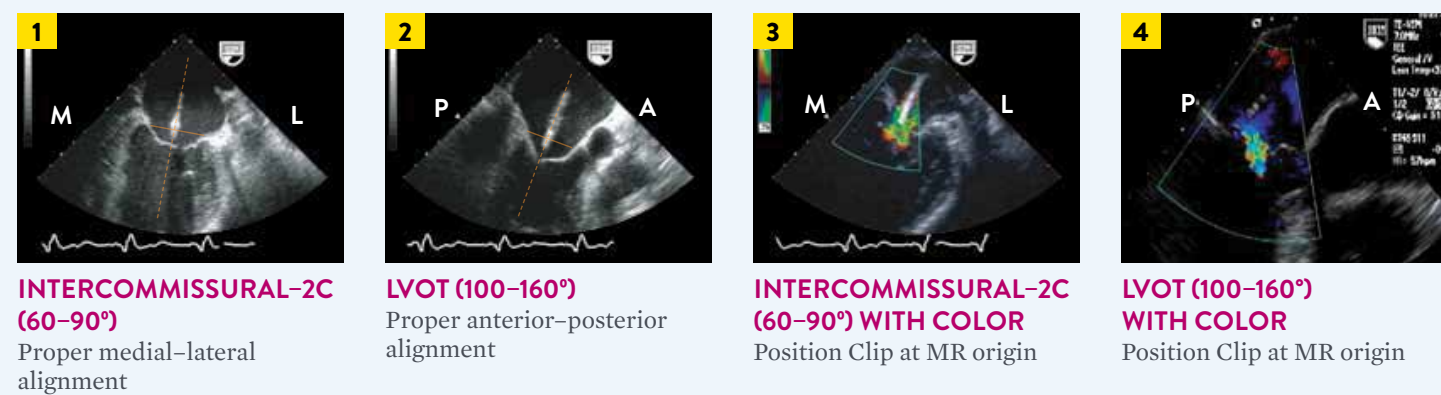

CLIP POSITIONING

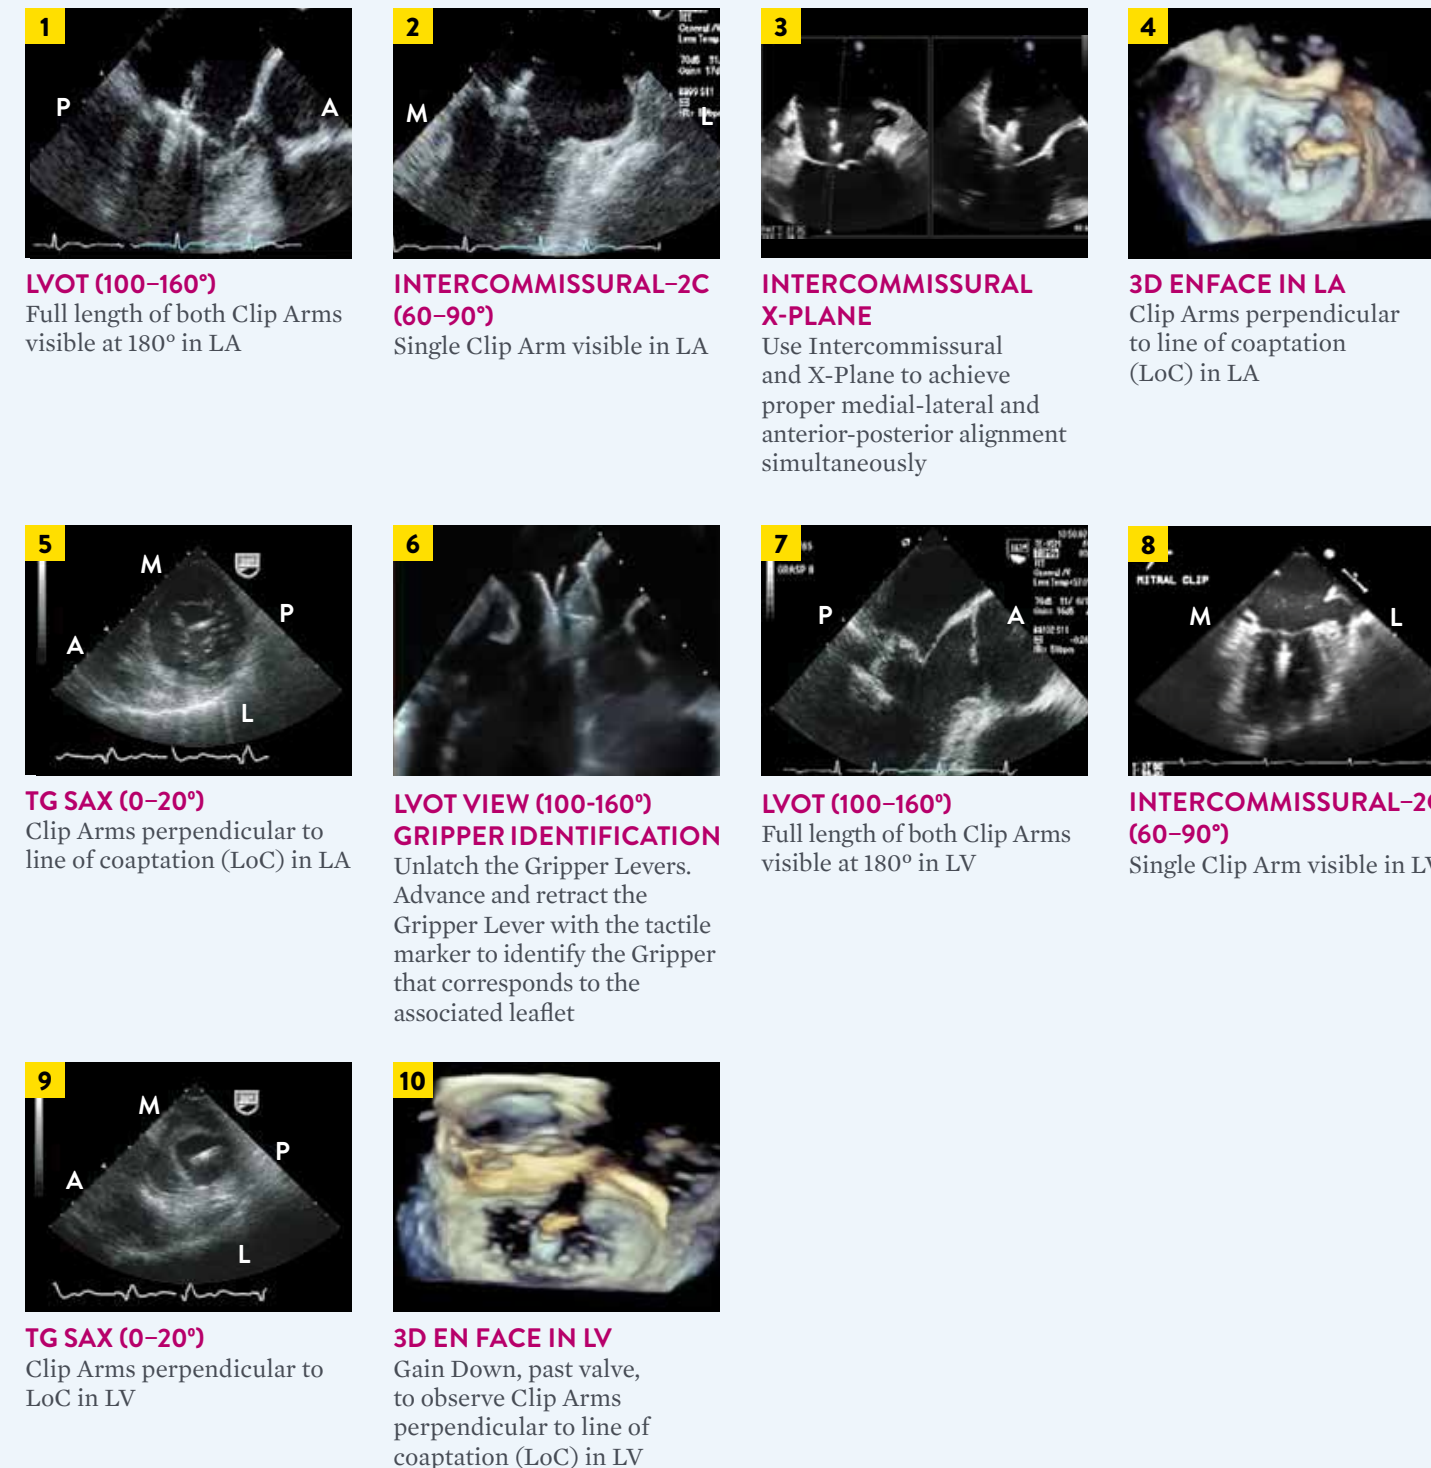

LEAFLET INSERTION ASSESSMENT

