


CardioMEMS™ HF System

PA Sensor and Delivery System

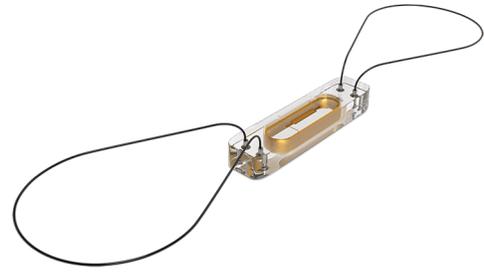

Product Highlights

- The CardioMEMS™ HF System is the fastest growing heart failure (HF) monitor proven to significantly reduce HF hospital admissions and improve quality of life in NYHA Class II and III patients.^{1,2} When used by clinicians to manage HF, the CardioMEMS HF System is:
 - **Safe and reliable** – demonstrates 99.6% freedom from device or system complications³
 - **Clinically proven** – reduced HF hospitalizations by 57%³
 - **Proactive and personalized** – patient management through direct monitoring of PA pressure and titration of medications
- The CardioMEMS HF System provides direct pulmonary artery (PA) pressure monitoring using the sensor, patient electronics system and the Merlin.net™ PCN website to manage patient data. Patient-initiated sensor readings are wirelessly transmitted to an electronics unit and stored in a secure website for clinicians to access and review
- The reliable radiopaque sensor is implanted in the pulmonary artery using a delivery system via a safe and proven right-heart catheterization procedure⁴
- In a prospective trial of 1,200 patients there was only one sensor failure reported (inability to obtain readings), indicating reliable PA pressure monitoring with only 0.1% failure.³
- The sensor endothelializes, occupying on average ~10% of cross-sectional lumen for low risk of infection, thrombus or occlusion⁵
- PA sensor pressure measurements (n = 85) showed agreement within $1.0 \pm .7$ (mean difference +/- sd) mmHg with a pulmonary artery catheter during follow-up measurements performed after an average follow-up of 265 ± 169 days post implantation without interim re-calibration⁶
- The sensor is calibrated during manufacturing and the mean pressure baseline is matched to the pulmonary artery catheter mean pressure during the implant procedure. The sensor does not contain a battery or other components which would limit its usable life

Ordering Information

Contents: PA Sensor and Delivery System

| MODEL NUMBER | DESCRIPTION |
|--------------|-------------------------------|
| CM2000 | PA Sensor and Delivery System |

1. Lindenfeld J, Zile MR, Desai AS, et al. Haemodynamic-guided management of heart failure (GUIDE-HF): a randomised controlled trial. *Lancet*. 2021;398(10304):991-1001. doi:10.1016/S0140-6736(21)01754-2

2. Brugts JJ, Radhoe SP, Clephas PRD, et al; MONITOR-HF Investigators. Remote haemodynamic monitoring of pulmonary artery pressures in patients with chronic heart failure (MONITOR-HF): a randomised clinical trial. *Lancet*. 2023;401(10394):2113-2123. doi:10.1016/S0140-6736(23)00923-6

3. Shavelle DM, Desai AS, Abraham WT, et al. Lower rates of heart failure and all-cause hospitalizations during pulmonary artery pressure-guided therapy for ambulatory heart failure: one-year outcomes from the CardioMEMS post-approval study. *Circ Heart Fail*. 2020;13(8):e006863. doi:10.1161/CIRCHEARTFAILURE.119.006863

4. Abraham WT, Adamson PB, Bourge RC, et al. Wireless pulmonary artery haemodynamic monitoring in chronic heart failure: a randomised controlled trial. *Lancet*. 2011;377(9766):658-666. doi:10.1016/S0140-6736(11)60101-3

5. Abbott. Data on File. G060187, September 2006. PMA P100045, December 2010. G060187/S031, August 2008.

6. Abbott. Data on File. The CardioMEMS Champion™ HF Monitoring System for Patients with NYHA Class III Heart Failure: Draft Briefing Document for the Circulatory Systems Device Panel Advisory Committee. December 8, 2011. P100045.


CardioMEMS™ HF System

PA Sensor and Delivery System

HEART FAILURE MONITORING SYSTEM


Product Specifications

| | |
|--|---|
| Model | CM2000 |
| CardioMEMS™ PA Sensor | |
| Sensor Body Dimensions (H x W x D, mm) | 2 x 3.4 x 15 |
| Wire Loop Expanded Diameter (mm) | 10 |
| Total Length (including wire loops) (mm) | 45 |
| Longevity | Permanent implant |
| Power | |
| Power Source | Externally powered by radiofrequency energy |

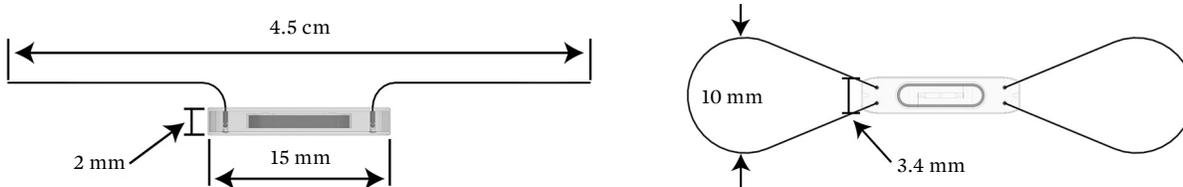

CardioMEMS™ PA Sensor Delivery System

| | |
|------------------------------------|--------------------------------|
| Model | CM2000 |
| Electronics Unit | |
| Delivery System Usable Length (mm) | 1200 |
| Guidewire Lumen | 0.018" (0.46 mm) OD Guidewires |
| Compatibility | 12 F sheaths |

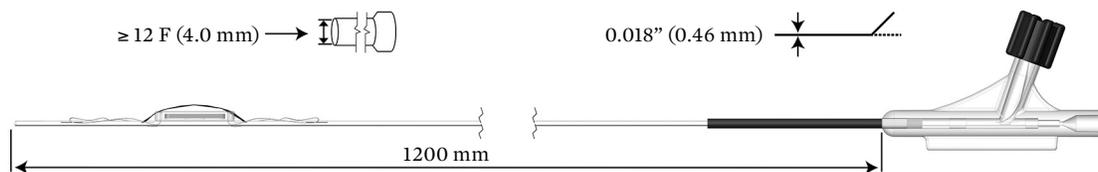

Abbott

6101 Stoneridge Dr., Pleasanton, CA 94588 USA, Tel: 1 925 847 8600
Cardiovascular.Abbott/CardioMEMS

Rx Only

Brief Summary: Prior to using these devices, please review the Instructions for Use for a complete listing of indications, contraindications, warnings, precautions, potential adverse events and directions for use.

CardioMEMS™ HF System Indications and Usage: The CardioMEMS™ HF System is indicated for wirelessly measuring and monitoring pulmonary artery pressure and heart rate in NYHA Class II or III heart failure patients who either have been hospitalized for heart failure in the previous year and/or have elevated natriuretic peptides. The hemodynamic data are used by physicians for heart failure management with the goal of controlling pulmonary artery pressures and reducing heart failure hospitalizations.

CardioMEMS™ HF System Contraindications: The CardioMEMS HF System is contraindicated for patients with an inability to take dual antiplatelet or anticoagulants for one month post implant.

CardioMEMS™ HF System Potential Adverse Events: Potential adverse events associated with the implantation procedure include, but are not limited to, the following: air embolism, allergic reaction, infection, delayed wound healing, arrhythmias, bleeding, hemoptysis, hematoma, nausea, cerebrovascular accident, thrombus, cardiovascular injury, myocardial infarction, death, embolization, thermal burn, cardiac perforation, pneumothorax, thoracic duct injury and hemothorax.

™ Indicates a trademark of the Abbott group of companies.

‡ Indicates a third-party trademark, which is property of its respective owner.

© 2025 Abbott. All Rights Reserved.

MAT-2009720 v4.0 | Item approved for U.S. use only.

