
EARLY TREATMENT IS ESSENTIAL

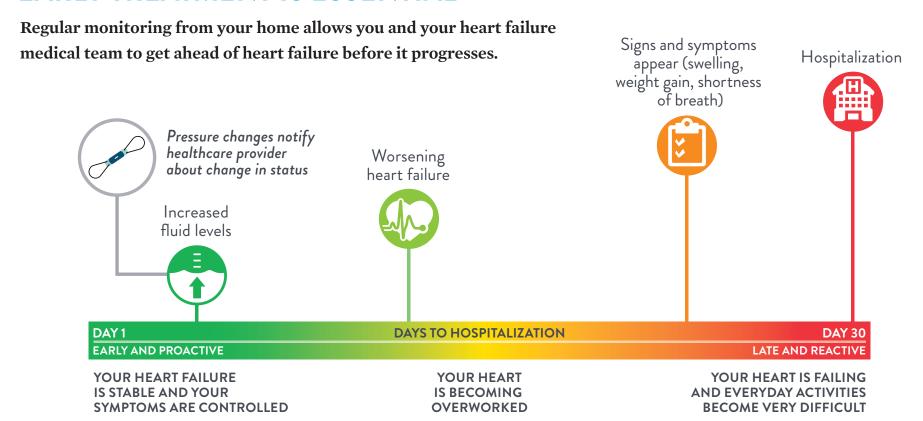

A study found that with each subsequent heart failure-related admission, the patient leaves the hospital with a further decrease in cardiac function and heart failure prognosis worsens dramatically.¹

In a clinical study of heart failure patients,* the CardioMEMS™ HF System led to a/an:

SIGNIFICANT


IMPROVEMENT IN

QUALITY OF LIFE²

INCREASE IN
SIX-MINUTE
WALK DISTANCE³

REDUCTION INHEART FAILURE
HOSPITALIZATIONS²

STAY AHEAD OF HEART FAILURE AT HOME

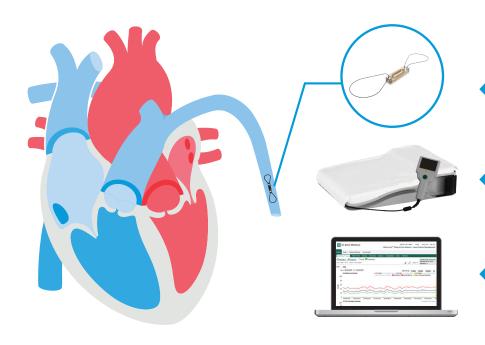

How the CardioMEMS™ HF System works

Sensor is inserted using a common procedure.

You simply take a 2–3 minute daily measurement of the sensor from the comfort of your home.

Your healthcare provider reviews your information and contacts you when necessary.

*In the CHAMPION clinical trial (CardioMEMS Heart Sensor Allows Monitoring of Pressures to Improve Outcomes in NYHA Class III Heart Failure Patients), patients with moderate (NYHA Class III) heart failure for at least three months, irrespective of left ventricular ejection fraction, and a heart failure hospitalization within the past 12 months were included in the study.

- Bui AL, Horwich TB, Fonarow GC.
 Epidemiology and risk profile of heart failure.
 Nature Reviews Cardiology. 2011;8(1):30-41.
- Abraham WT, Stevenson LW, Bourge RC, Lindenfeld JA, Bauman JG, Adamson PB, for the CHAMPION Trial Study Group. Sustained efficacy of pulmonary artery pressure to guide adjustment of chronic heart failure therapy: complete follow-up results from the CHAMPION randomised trial. *The Lancet*. 2016;387(10017):453-461.
- 3. Alam A, Jermyn R, Joseph M, Patel S, Jorde U, Saeed O. Improved quality of life scores and exercise capacity with remote pulmonary artery pressure monitoring in patients with chronic heart failure. *Journal of the American College of Cardiology*. 2016;67(13):1299.

Abbott

The Corporate Village, Da Vincilaan 11 Box F1 1935 Zaventem, Belgium Tel: +32 2 774 68 11 SJM.com St. Jude Medical is now Abbott.

Brief Summary: Prior to using these devices, please review the Instructions for Use for a complete listing of indications, contraindications, warnings, precautions, potential adverse events and directions for use.

™ Indicates a trademark of the Abbott group of companies.© 2018 Abbott. All Rights Reserved. 29313-SJM-MEM-0518-0418a Information contained herein for DISTRIBUTION outside of the U.S. ONLY. Check the regulatory status of the device in areas where CE marking is not the regulation in force.

